This Page Is Inserted by IFW Operations and is not a part of the Official Record

BEST AVAILABLE IMAGES

Defective images within this document are accurate representations of the original documents submitted by the applicant.

Defects in the images may include (but are not limited to):

- BLACK BORDERS
- TEXT CUT OFF AT TOP, BOTTOM OR SIDES
- FADED TEXT
- ILLEGIBLE TEXT
- SKEWED/SLANTED IMAGES
- COLORED PHOTOS
- BLACK OR VERY BLACK AND WHITE DARK PHOTOS
- GRAY SCALE DOCUMENTS

IMAGES ARE BEST AVAILABLE COPY.

As rescanning documents will not correct images, please do not report the images to the Problem Image Mailbox.

APPLN. FILING DATE: JANUARY 30, 2004
TITLE: BLOOD PRESSURE MEASURING APPARATUS INVENTOR(S): GÖTZ, PETER ET AL APPLN. SERIAL NO.: SHEET 1 OF 5

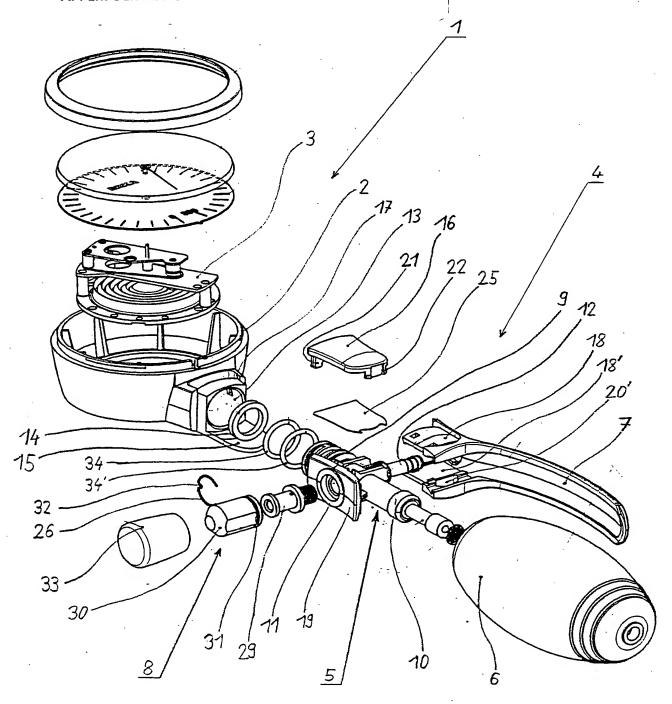


Fig. 1

APPLN. FILING DATE: JANUARY 30, 2004
TITLE: BLOOD PRESSURE MEASURING APPARATL
INVENTOR(S): GÖTZ, PETER ET AL
APPLN. SERIAL NO.: SHEET 2 OF 5

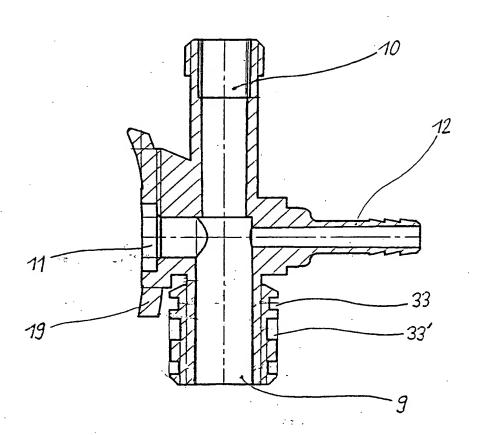


Fig. 2

APPLN. FILING DATE: JANUARY 30, 2004
TITLE: BLOOD PRESSURE MEASURING APPARATUS
INVENTOR(S): GÖTZ, PETER ET AL
APPLN. SERIAL NO.: SHEET 3 OF 5

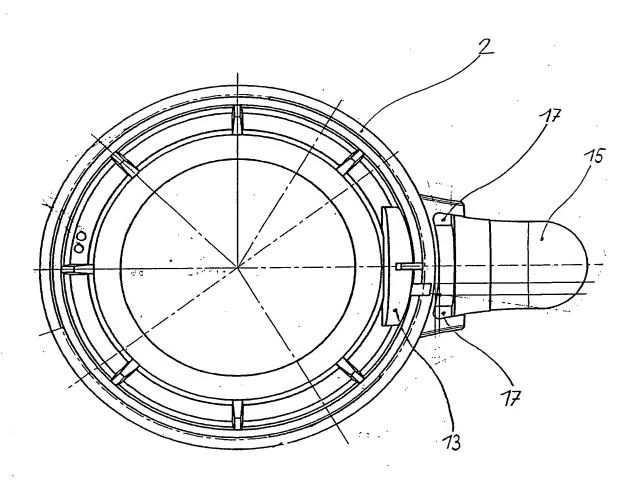


Fig. 3

APPLN. FILING DATE: JANUARY 30, 2004
TITLE: BLOOD PRESSURE MEASURING APPARATL
INVENTOR(S): GÖTZ, PETER ET AL
APPLN. SERIAL NO.: SHEET 4 OF 5

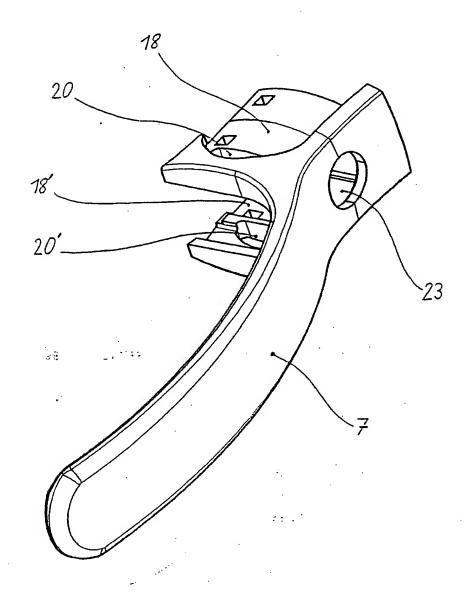
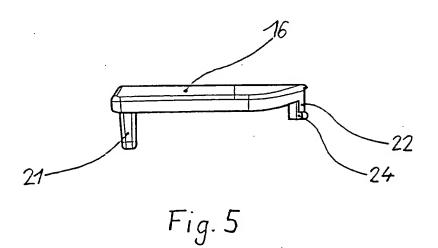


Fig. 4

APPLN. FILING DATE: JANUARY 30, 2004
TITLE: BLOOD PRESSURE MEASURING APPARATUS
INVENTOR(S): GÖTZ, PETER ET AL
APPLN. SERIAL NO.: SHEET 5 OF 5



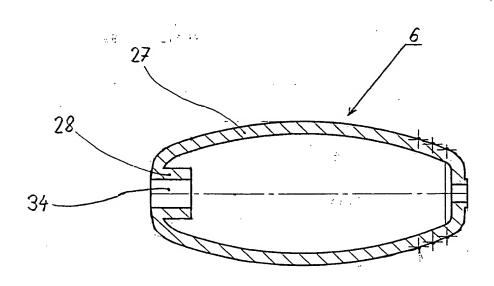


Fig. 6